Installation instruction

Network Isolator MED MI 1005 MB

▸ Bill of Material (BOM)

Please check the BOM prior to assembling the parts.

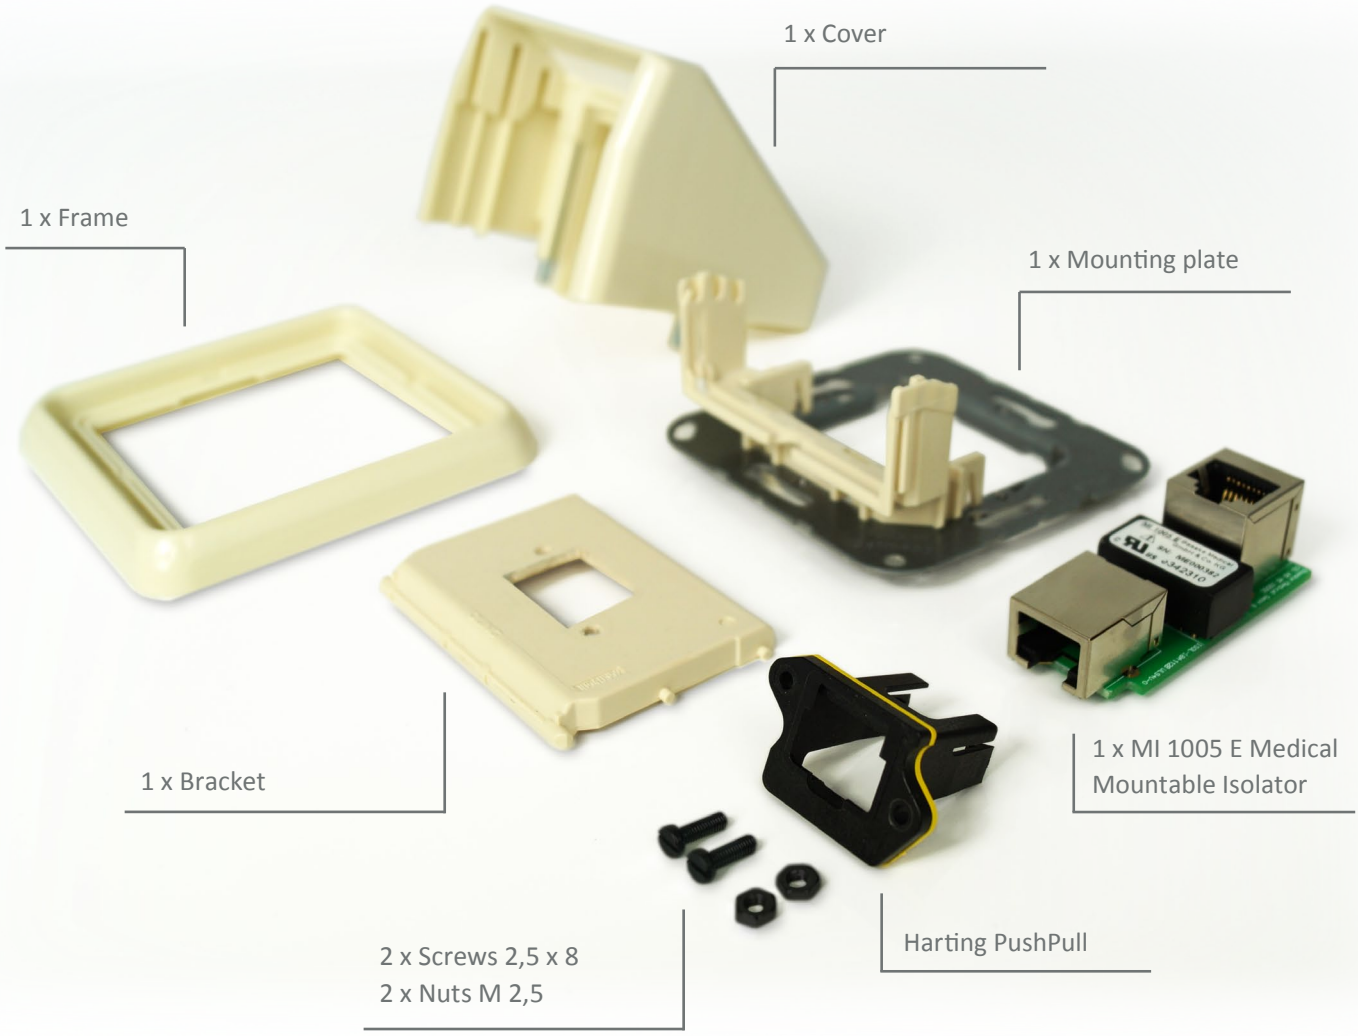
1 x Cover
1 x Frame
1 x Mounting plate
1 x Bracket
1 x MI 1005 E Medical Mountable Isolator
2 x Screws 2,5 x 8
2 x Nuts M 2,5
Harting PushPull

Changes and errors excepted.

Baaske Medical GmbH & Co. KG ▸ Bacmeisterstraße 3 32312 Lübbecke ▸ Tel: +49 5741 236027- 0 ▸ Fax: +49 5741 236027- 99
www.baaske-medical.de

Installation

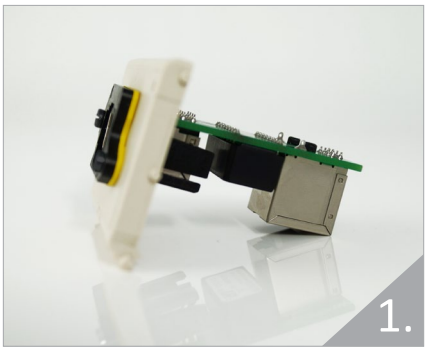

1. Fix the Harting PushPull with the provided bracket, using screws and nuts included the package. Than snap the MI 1005 E Medical Mountable Isolator with the black bracket.

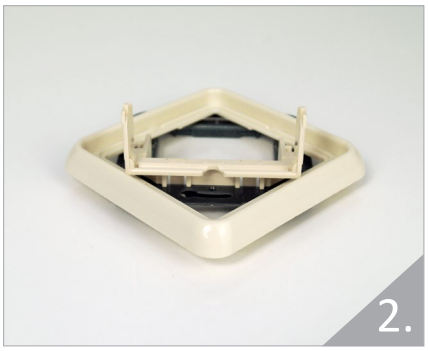

2. Cover the mounting plate with the frame part.

3. Move the frame until it fits correctly.

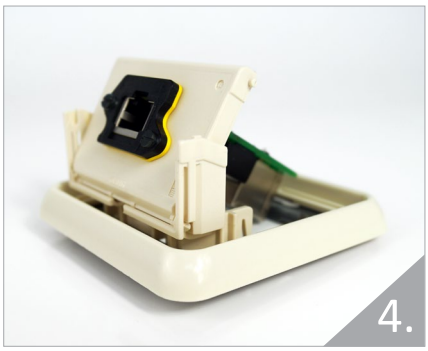

4. Insert the pre-assembled bracket angled into the mounting plate. Make sure that the RJ45 Socket is accessible.

5. Put the cover on the mounting plate and attach it securely. The cover must fit properly into the framework below.

6. Print and attach the labl cover.

Changes and errors excepted.

Baaske Medical GmbH & Co. KG ▸ Bacmeisterstraße 3 32312 Lübbecke ▸ Tel: +49 5741 236027- 0 ▸ Fax: +49 5741 236027- 99
www.baaske-medical.de